

RADIATION-HARDENED MAGNETS USING MINERAL-INSULATED CONDUCTORS*

A. Harvey
Los Alamos Scientific Laboratory, University of California
Los Alamos, New Mexico

Abstract

A unique feature of the LAMPF high-intensity linac experimental area is the extensive use of inorganic magnet coils to withstand the high radiation doses expected.

The coil insulation is compacted magnesium oxide powder ("mineral insulation," m.i.) and pre-insulated cable is wound into the required coil configuration. Although the cable itself is expensive compared to bare copper conductor, the finished coil cost is comparable to a conventional coil, since no insulation application is required of the coil winder.

Two conductor formats are used at LAMPF: solid conductor, externally cooled, using soft solder to improve the heat transfer within the coil; and directly cooled, hollow conductor m.i. cable. At LAMPF both conductor types are conservatively rated. Indirectly cooled coils are used exclusively in the switchyard magnets, where low field strengths and high quality are required. Higher-power magnets for target-to-target transport and secondary beam lines use direct cooling. Methods of making terminations on the cable are described.


Measured operating parameters for all these magnets are tabulated. Pole-shaping techniques for the bending magnets and quadrupoles are examined and the results given.

I. Introduction

One of the dominant problems facing the designers of the LAMPF experimental area, and beam handling facilities, was the anticipated high radiation dose arising from the high intensity of the beam. The 1 mA average current of 800 MeV protons impinging on a target such as graphite or molybdenum is expected to produce radiation doses in the target cells of 10^{11} - 10^{12} rad/yr. "Conventional" magnet insulations (such as epoxy-fiberglass, with a radiation tolerance of 10^{10} rad max) were ruled out, and after some consideration, "mineral-insulation" was decided on.

"Mineral-insulation" is a term from the wire and cable industry, used to describe an electrical insulation of metal oxide (usually magnesium oxide). The oxide is in the form of a powder, generally held around the copper conductor by a copper sheath (see Fig. 1). Although multiple

conductor formats are common in the industry, only one conductor is required for magnet coil fabrication. The development needed was to make the cable square, to improve packing in a coil, and to provide direct conductor cooling for higher current densities.

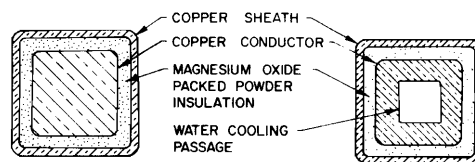

MINERAL INSULATED
SOLID CONDUCTOR
CABLE

MINERAL INSULATED
HOLLOW CONDUCTOR
CABLE

FIG. 1

This paper illustrates the successful achievement of these objectives. It should be noted that at present there are only two plants in North America with the capability of producing the cables described here: Pyrotanax of Canada Ltd., in Trenton, Ontario, Canada, and General Cable Corp. in Perth Amboy, N.J. All of the m.i. cable used at LAMPF has been produced by Pyrotanax of Canada Ltd.

II. Cable

Formats

Two formats of mineral-insulated cable are used at LAMPF. The solid conductor cable is a single-conductor cable of conventional construction, formed square outside, and used with external cooling (indirect cooling).

Hollow conductor cable has a hole in the center of the conductor to allow direct water cooling, and hence, higher current densities (Fig. 1). This is a rather significant change in the usual manufacturing process for mineral-insulated cable, but has been done before.¹

Manufacture

General

Two manufacturing methods are currently

*Work performed under the auspices of the U.S. Atomic Energy Commission.

employed to produce m.i. cable commercially. In the first method, short tubular preforms of magnesium oxide are pressed and baked, and then loaded into the annulus between the conductor rod and sheath tube. In this case the reduction in cross section by drawing is generally not great (about 50% in diameter in several draws). Each one or two draws is followed by an annealing cycle to soften the copper.

The second method fills the annulus between the conductor rod and sheath tube (the latter about 2" o.d.) with MgO powder, tamped firmly in an assembly up to 30 ft long. This then is reduced to the required size (with anneals as necessary between draws). In either method square cable is produced by using square dies instead of the usual circular ones for the final draws.

The maximum length of cable that can be manufactured is set generally by the length of the assembly at the start, and the annealing furnace used when the cable cannot be coiled, since later draws use a bull-block, coiling up the cable, and so are capable of handling any length of cable. Current technology gives the edge on length to the powder-fill method; and Table 1 lists the lengths now available.

TABLE 1.
Maximum Available Lengths
for Mineral-Insulated Cable

Solid		Hollow	
Nominal Size	Maximum Length	Nominal Size	Maximum Length
0.25" sq	1,000 ft	0.375" sq	400 ft
0.375" sq	700 ft	0.53" sq	220 ft
0.412" sq	650 ft	0.75" sq	220 ft
0.53" sq	420 ft		

Solid Conductor

Solid conductor m.i. cable for magnet use is basically a standard round, single-conductor, mineral-insulated cable. However, the insulation thickness required by the conservative electrical licensing authorities for use in 600V rated power wiring is more than a magnet designer needs, since it reduces his packing factor and the magnet voltage generally does not exceed 200V. To date we have succeeded in providing minimal insulation thickness only in the 0.25" sq size (see Table 1). Given sufficient inducement there is no doubt the manufacturer could do the same in the other sizes.

Specifications for the three sizes of solid-conductor m.i. cables used at LAMPF are given in Tables 2 through 4. The pertinent comment here is that the 0.412" square and 0.53" square sizes

are standard circular, single-conductor m.i. cables drawn square. However, the 0.25" sq size requires a special manufacturing process (note the packing factor for this size is 32%, quite good for such a small conductor).

TABLE 2.
Mineral Insulated Solid
Conductor Cable, 0.25" Sq.

Specification: Overall size: 0.250" sq + 0.000" - 0.010"
Corner radius 0.050" max
Conductor size: 0.157" nominal square outside
Insulation thickness: 0.015" minimum
0.020" nominal
Sheath thickness: 0.020" + 0.005" - 0.00"

Materials: Conductor: copper, 100% I.A.C.S.
Max. resistance at 25°C: 0.4 Ω/1000 ft
Insulation: compacted magnesium oxide
Sheath: copper, commercial anneal.
Free of burrs, nicks and scratches.

Tests: Insulation resistance, inner conductor to outer sheath > 5,000 MΩ/1000 ft at 25°C, 100V dc
Dielectric strength, > 1,250V rms inner conductor to sheath, 1 min
Immersion of coiled cable (except ends) in warm water for 30 min to produce no change in insulation resistance.

Weight: 180 lb/1,000 ft
Nominal current rating: 125A
Shipping: Coiled to minimum diameter of 4 ft.
All ends of insulation sealed against moisture.

TABLE 3. Mineral Insulated Solid
Conductor, Cable 0.412" Sq.

Specification: Overall size: 0.412" sq + 0.000" - 0.010"
Corner radius 0.032" max
Conductor size: 0.238" nominal square outside
Insulation thickness: 0.030" minimum
0.060" nominal
Sheath thickness: 0.027" ± 0.005"

Materials: Conductor: copper 100% I.A.C.S.
Resistance: 0.159 Ω/1000 ft nominal
0.169 Ω/1000 ft maximum
Insulation: compacted magnesium oxide
Sheath: copper, commercial anneal,
free of nicks, scratches and burrs

Tests: Insulation resistance, inner conductor to outer sheath > 5,000 MΩ/1000 ft at 25°C, 100V dc
Dielectric strength > 1,500V rms inner conductor to sheath, 1 min
Immersion of coiled cable (except ends) in warm water for 30 min to produce no change in insulation resistance

Weight: 425 lb/1,000 ft
Shipping: See Table 2.
Nominal current rating: 180A

TABLE 4. Mineral Insulated Solid Conductor Cable 0.53" Sq.

Specification: Overall size: 0.530" sq + 0.000" - 0.010"
 Corner radius 0.032" max
 Conductor size: 0.350" nominal square outside
 Insulation thickness: 0.030" minimum
 0.060" nominal
 Sheath thickness: 0.030" ± 0.005"
 Materials: Conductor: copper 100% I.A.C.S.
 Resistance: 0.0795 Ω/1000 ft nominal
 0.0844 Ω/1000 ft maximum
 Insulation: compacted magnesium oxide
 Sheath: copper, commercial anneal,
 free from nicks, scratches
 and burrs
 Tests: Insulation resistance, inner conductor to
 outer sheath > 5,000 MΩ/1000 ft at 25°C,
 100V dc
 Dielectric strength > 1,500V rms inner
 conductor to sheath, 1 min
 Immersion of coiled cable (except ends)
 in warm water for 30 min to produce no
 change in insulation resistance
 Weight: 726 lb/1000 ft
 Shipping: Coiled to minimum diameter of 4 ft.
 All ends of insulation sealed against
 moisture.
 Nominal current rating: 300A

Hollow Conductor

To enable direct water-cooling of the conductor, a hole is required in the center of the conductor. Again, two methods are available to produce this: using a die in the bore (either fixed or floating), or filling the bore of the conductor to prevent its collapse during drawing. This latter method requires the filling to be easily removable for annealing and final use. Again, lengths available are listed in Table 1. Specifications for two sizes are given in Tables 5 and 6.

Tests

Electrical. The electrical characteristics of the cable are of paramount importance, and in fact, because of the inherently irregular configuration of the conductor, are specified in preference to mechanical dimensions. It should be clear that the outside dimensions of the cable, being produced by drawing, can be held to close tolerances. However, the conductor itself is formed by the intermediate MgO layer, and the outside and inside of the conductor are difficult to define in dimensional terms.

It is more reasonable, then, to define (1) a conductor maximum resistance (which controls both the cross-sectional area and the copper quality), (2) an insulation resistance between conductor and sheath, which controls the quality (mainly dryness) of the magnesium oxide insulation, and (3) a high-potential test, which controls the minimum insulation thickness. Tables 2 - 6 give examples of such specifications.

TABLE 5. Mineral Insulated Hollow Conductor Cable 0.53" Sq.

Specification: Overall size: 0.530" sq + 0.000" - 0.010"
 Corner radius 0.063" maximum
 Conductor size: 0.36" nominal square outside
 0.18" nominal square inside
 0.050" minimum wall thickness
 Insulation thickness: 0.020" minimum
 0.055" nominal
 Sheath thickness: 0.030" ± 0.005"
 Materials: Conductor, copper, 100% I.A.C.S.
 Max resistance at 25°C: 0.091 Ω/1000 ft
 Insulation, compacted magnesium oxide
 Sheath, copper, commercial anneal
 Tests: Insulation resistance, inner conductor to
 outer sheath > 5,000 MΩ/1000 ft at 25°C,
 100V dc
 Dielectric strength, > 1,500V rms inner
 conductor to sheath, 1 min
 Water tests: 300 psi water in central
 hole to produce no change in insulation
 resistance
 Immersion of coiled cable (except ends)
 in warm water for 30 min to produce no
 change in insulation resistance
 Water flow: 0.5 USGPM, with max pressure drop
 1.0 psi/ft
 Weight: 0.6 lb/ft
 Shipping: Coiled to minimum diameter of 4 ft.
 All ends of insulation sealed against
 moisture. Tube ends plugged.
 Nominal current rating: 750A

TABLE 6. Mineral Insulated Hollow Conductor Cable, 0.75" Sq.

Specification: Overall size: 0.75" sq + 0.00" - 0.01"
 Corner radius: 0.08" max
 0.04" min
 Conductor size: 0.57" nominal square outside
 0.26" nominal square inside
 0.09" min wall thickness
 Insulation thickness: 0.05" nominal
 0.03" minimum
 Sheath thickness: 0.035" ± 0.005"
 Materials: Conductor: copper 100% I.A.C.S.
 Max resistance at 25°C: 0.035 Ω/1000 ft
 Insulation: compacted magnesium oxide
 Sheath: copper, commercial anneal
 Tests: Insulation resistance, inner to outer >
 5,000 MΩ/1000 ft at 25°C, 100V dc
 Dielectric strength, > 1,500V rms inner
 conductor to sheath, 1 min
 Water test: 400 psi water in central hole
 to produce no change in insulation
 resistance
 Water flow: 2.5 USGPM, with max pressure drop
 200 psi/180 ft
 Weight: 1.4 lb/ft
 Nominal current rating: 1800A
 Shipping: Coiled to minimum diameter of 4 ft.
 All ends of insulation sealed against
 moisture. Tube ends plugged.

Mechanical. Arguments similar to those above lead to very few mechanical parameters being specified. The outside dimensions are given, with low-side tolerances only, for convenience. A corner radius is desirable to reduce the tendency to crack at bends.

Conductor lengths are chosen to suit the particular design: the maxima for various sizes are listed in Table 1.

Hydraulic. The hydraulic tests serve two purposes: to insure adequate cooling flow, and to insure the integrity of the sheath and conductor wall.

The water-flow test specifies a maximum pressure drop for the flow required to maintain cooling at the rated current, and controls the cross section of the cooling passage. It may be noted that, again, this hole may be irregular; the common practice of blowing a ball through the cooling passage is not recommended with m.i. cable.

Two tests check the integrity of the copper enclosing the MgO insulation. An immersion in water tries the outer sheath, while pressurizing the cooling passage with water checks the conductor wall. Measuring insulation resistance after these tests determines if there has been any water penetration into the MgO. This test is extremely sensitive, since the loss of insulation resistance caused by moisture is catastrophic.

III. Coils

General

The manufacture of coils from m.i. cable is generally similar to conventional techniques, with the main difference being that no insulation application is required. Coil forms are standard, and tension is applied in the usual way. The relatively long lengths in which m.i. cable is available makes joining generally unnecessary: LASL practice has been to make terminations and external joints when the lengths are not adequate. An advantage of this system is that, in case of insulation problems for instance, individual sections can be isolated and tested.

A parameter of interest in coil design and fabrication is the minimum bending radius. There are two criteria which can be used: the first, within a coil, is the amount of "keystoning" which is produced; and the second (on leads, for example) is simply the smallest radius which will not damage the cable sheath. Both criteria are listed in Table 7.

It must be stressed that, in bending the conductor outside a coil, particularly to minimum radius, a mandrel and bending fixture are necessary. The copper sheath is soft and less than 0.004" thick, and can be damaged by local pressure.

TABLE 7.

Cable Size	In-coil		Out-of-Coil
	Min. Radius	Keystoning	Min. Radius
0.25" sq	0.9"	0.010"	0.6"
0.375" sq	1.1"	0.012"	0.75"
0.412" sq	1.25"	0.010"	1"
0.53" sq	1.75"	0.02"	1.5"
0.75" sq	2.5"	0.02"	2"

Indirectly-Cooled Coils

For magnets requiring low power densities (at LAMPF, the switchyard magnets, where fields generally do not exceed 4 kG because of the H⁺ beam) it is feasible to use a solid-conductor cable, cooled externally, to wind coils. As has been pointed out previously², soft-soldering can be used to effect the heat transfer from conductor to cooling channels. This still seems the most economical way to provide the requisite metallic path for heat conduction: the quality of the soldering required is dependent on the heat transfer efficiency (and so, power density) required. One requirement we have found necessary is to insure that no corrosive flux remains in the final soldered assembly. We also require pre-tinning of the cable.

Since heat from the conductor traverses insulation only once before being transferred by the matrix of copper sheaths and solder to the cooling channels, relatively high current densities may be used. Table 8 gives, in addition to recommended current densities already published,² limiting current densities which will cause solder melting in 10-layer test coils, water-cooled on one side. Both these ratings depend on the quality of the soldering (i.e., the voids left in the coil).

TABLE 8.

Cond. Size	Recommended		Maximum	
	Current Density	Current	Current Density	"Solidus" Current
0.25" sq	5100 A/in ²	125A	11,800 A/in ²	290 A
0.412"sq	3200 A/in ²	180A	4,710 A/in ²	265A
0.53" sq	2450 A/in ²	300A	N/A	-

Soldering. There are a number of ways to solder the cable and cooling-coil assembly together. We outline three methods here, with their relative advantages and disadvantages, but three features are common to them all. 1) Tinning the cable

before (or during) winding is the only way to insure that solder wets the sheath inside the coil.

2) The coil dimensions have to be maintained during soldering. Steel banding straps will hold the coil cross section, and are easily removed after soldering, as the strap is not wet by solder.

3) Any corrosive flux must be excluded from the finished coil assembly. Since removal is difficult, the safest course is to solder the pre-tinned parts without using flux. This is quite practical if care is taken to avoid excessive oxidation of the tinning.

A. Dip Soldering. This requires a solder bath larger than the coil assembly to be soldered, so is probably the most expensive method of the three. Further, it is necessary to remove the coil from the bath at a temperature as close to the solidus point as possible, otherwise most of the solder simply runs out of the coil. It is difficult to provide void-free construction this way.

B. Casting. Here the coil assembly is placed in a mold and molten solder is poured in. Pre-heating of the coil seems desirable to insure penetration to the inside of the coil, but if this is done, this method produces the best filling of the coil, hence the maximum heat transfer.

C. Resistance Heating. The coil may be heated electrically (using the conductor) and solder applied from the outside, usually with the assistance of local torch (flame) heating. A chill plate on the bottom of the coil prevents excessive loss of solder (a cooling coil may be used as the chill plate). This is probably the cheapest method of soldering the coil, as no special equipment is required, but the quality of the job depends on the care which is taken, and some judgment is required of how much solder to add to the coil to fill most of the internal voids. However, for conservative ratings, such as are used at LAMPF, the results are perfectly satisfactory.


Terminations. The sealing of the MgO insulation (to keep moisture out) is a problem common to solid and hollow conductor m.i. cables. Since the radiation environment dictates the use of an inorganic insulation in the cable, non-organic seals are used at LAMPF. A fairly standard ceramic-to-metal seal (see Fig. 2) is squared at the larger end to fit the cable sheath. Nickel ends form relatively easy; Kovar may be formed if pressure is applied to all four sides simultaneously. The conductor is machined to a more circular cross section (by a hollow mill in a hand drill) and the seal is soldered in place. Two soldering techniques are used, both intended to keep flux from reaching the MgO insulation, which seriously and permanently degrades its insulation resistance.

1) Soft-Soldering

- a) Tin the ends of the ceramic-to-metal seal with 50-50 solder (flux permitted), wash in hot water and dry. Check insulation resistance and leak tightness.

NOTES

- 1. Silver brazed, vacuum tested by helium leak detector
- 2. Metal ends copper plated 0.0001 to 0.0005 thk. x 1/2 lg. min.

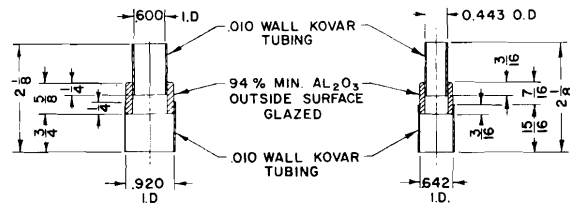

0.75 SQ. M.I. CABLE 0.53 SQ. M.I. CABLE

FIG. 2
CERAMIC SEALS

- b) Cut back the cable sheath to the required distance, clean copper slivers and dust from the MgO surfaces, and thoroughly clean the copper (wire brush).
- c) Put a temporary epoxy seal in the end of the MgO. We suggest Hysol 615 or Astrodyne Thermal-Bond 312.*
- d) Mill the conductor section exposed, and check that the seal fits.
- e) Tin an inch or two of cable sheath and adjacent conductor with 50-50 solder (flux permitted), wash and dry.
- f) Remove temporary epoxy seal completely and check cable insulation resistance. Dry out if necessary.
- g) Put seal in place and solder using no flux and a reducing torch flame. Build up a substantial layer of solder at both joints.
- h) Recheck cable insulation resistance and follow for a day or two for signs of moisture penetration.

2. Hard-Soldering

- a) Cut back the cable sheath to the required distance, clean copper slivers and dust from the MgO surface, and thoroughly clean the copper (wire brush).
- b) Put a temporary epoxy seal in the end of the MgO. We suggest Hysol 615 or Astrodyne Thermal-Bond 312.*

* The Hysol epoxy is fast-setting (3-5 min) but will not tolerate a warm cable. If the cable has been warmed (to drive out moisture) the Astrodyne epoxy can be applied satisfactorily: its drying time then is 1/4-6 hours depending on the temperature.

- c) Mill the conductor section exposed and check that the seal fits. Note that in this case the epoxy seal serves largely to avoid losing MgO powder from the annulus during this operation.
- d) Remove the epoxy seal completely and check the cable insulation resistance. Dry out if necessary.
- e) Put seal in place and braze ends to copper using AWS BCuP-5 (Silfos) using no flux.
- f) Recheck cable insulation resistance and follow for a day or two for signs of moisture penetration.

Note that although the second technique has fewer steps, it requires more skill of the operator since the higher melting point of the solder increases the risk of damaging the ceramic-to-metal seal.

The seals used at LAMPF are of simple, inexpensive design. They are available from a number of ceramic-to-metal seal manufacturers.* If high conductor temperatures or rapid changes in current are anticipated, which might cause relative movement between conductor and sheath, seals can be made with a flexible metal disc incorporated in the end, to minimize the stress on the ceramic.

There may also be situations where radiation-hardening of the seal is not necessary. Then an epoxy seal (similar to the pot seals provided by

m.i. cable manufacturers for circular power cable) may be used. Removal of the MgO for 1/8" from the end, and filling this space with epoxy well bonded to the conductor and sheath provides a seal of good strength. A piece of 1" i.d. copper tubing, an inch long, can be squared for 1/2" and used as a pot on the 0.75 in. sq cable.

All seals require that care be taken in subsequent handling or manipulation of the cable end to avoid mechanical damage. At LASL seal installation is an in-house operation, and one of the last to be performed on the magnet.

Directly-Cooled Coils

Winding. Techniques for winding hollow m.i. cable are again quite conventional apart from insulation application. It is desirable to keep the conductor bore sealed to prevent foreign material entering the coolant passage, and, as with all operations on m.i. cable, the MgO should be sealed.

Cooling Connections. Directly-cooled conductors require insulating connections to water headers and to replace the rubber or synthetic hoses used in conventional magnets, we install ceramic water insulators. Figure 3 shows two sizes. These are designed to provide a long water path of minimal cross section to keep the leakage current through the water low (a radiation environment will decrease the water resistivity even though a high initial value -- 1 MΩ-cm at LAMPF -- is maintained). There is reason to believe that deposition of contaminants inside the insulator (generally copper oxide) is more dependent on the total voltage across the insulator than on the voltage gradient, 4

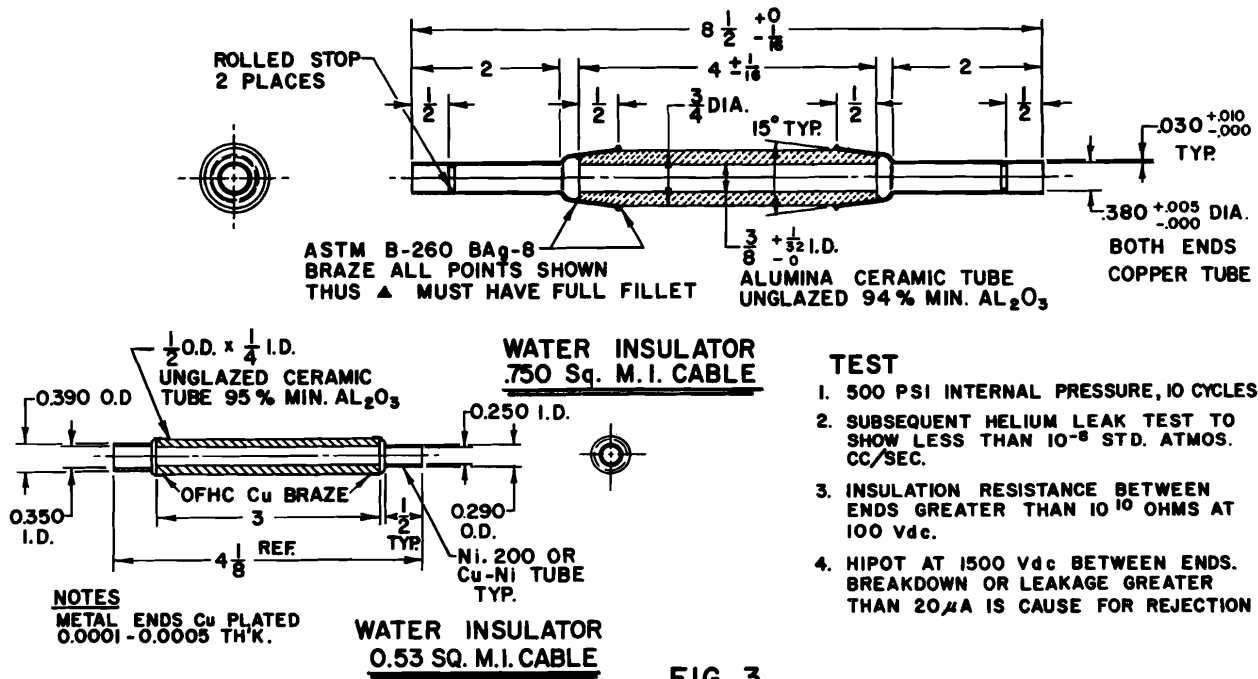


FIG. 3

*Alberox, Ceramaseal, Latronics, R & W Products

so the short lengths of these ceramic tubes compared to hoses may not be a great disadvantage.

To evaluate the possible problems in a radiation environment an assembly of two of these insulators (3" long x 1/4" i.d. Al_2O_3 tube in Fig. 3) was irradiated in LASL's Omega West Reactor. Each insulator was in a 300 psi water circuit with 100V dc across it. After a total radiation dose of 5×10^{11} rad the insulation resistance of these insulators had dropped from $> 5T\Omega$ to 0.7 and $1.7G\Omega$ respectively. There was some internal deposit on the ceramic tube, but obviously they were still adequate insulators.

The connections from conductor to insulator, and insulator to manifold, are made with annealed copper tubing. Two bends in orthogonal planes provide adequate strain relief for the ceramic tube, but we also put a tube fitting at each end of the insulator assembly to facilitate replacement. Figure 4 is a photograph of an 8" quadrupole with these insulators installed.

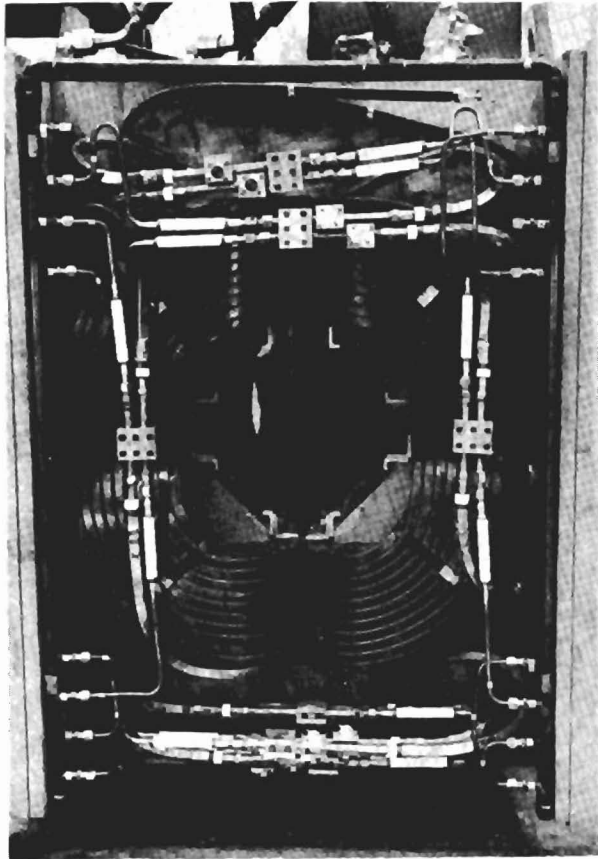


Fig. 4. 8QN16M/7 quadrupole with seals and insulators installed.

Repairs

Since damage to coils in fabrication or assembly seems inevitable, it is worthwhile to say something of repair techniques. Any penetration of the outer copper sheath allows ingress of atmospheric moisture, and the insulation resistance of the cable drops. Note that the moisture penetration into the MgO is slow, because of the tight packing, and is limited by the conversion of MgO to $\text{Mg}(\text{OH})_2$, with an increase in volume. This limits the moisture penetration from any exposed insulation to a foot or so. However, if the exposure to moisture has been long enough to form magnesium hydroxide, the cable has to be heated to 350°C minimum to drive off the water.

Diagnostics. A hole in the cable sheath can be found, if the cable insulation resistance is reasonably high, say over $10M\Omega$, by wetting the sheath locally. A wet cloth or spray bottle is convenient. A continuously-reading megohmmeter on the cable will show a marked decrease in I.R. when the water enters the hole -- and the effect is immediate.

However, probably a better test is to use a medium-sized oxy-acetylene torch flame, because this will provide an indication on the megohmmeter whatever the initial I.R. is (in fact, if it is below the megohm range, an ohmmeter may be used). The cable requires to be warmed only slightly, and an indication will be noted on the meter when the flame hits a moist patch in the cable.

Repair. Faced with a hole in the sheath, we have two possible courses of action. For a small hole less than $1/16$ " in any direction, it may be sealed using AWS BCuP-5 (Silfos) with no flux. This may be filed to give a flush surface. But larger holes require a patch of copper foil, again brazed on without flux. Trying to cover a large hole directly with Silfos generally results in the torch flame blowing MgO from the cable, so that the braze metal either contacts, or is very close to, the conductor, and no dielectric remains. In contrast, the space behind a patch may be packed with dry MgO powder and the final cable properties are unaffected. The outside dimensions, however, are increased.

Similar techniques are used to produce cable splices as illustrated in Ref. 2. In every case the vital point is to avoid contaminating the MgO insulation.

Specifications

It has been LASL practice to specify the wound coil tests as follows:

1. Insulation Resistance. A value $1/10$ of the cable "as supplied" resistance. For a typical 200 ft piece of cable, the cable manufacturer's

specification calls for $25G\Omega$, so the coil winder is required to maintain $2\frac{1}{2}G\Omega$ in the finished section. Note that in a magnet with 16 coil sections, this will give a completed magnet ground resistance of $156M\Omega$ minimum, which is generally more than sufficient for any leakage or regulation requirements. Discretion may be used to drop the minimum acceptable insulation resistance.

2. Hipot Test. The coil high-potential test is specified as 1500V dc, giving an applied voltage 0.7 times that used for the cable.

3. Water Flow. The same maximum pressure drop for the required water flow rate is specified for the coil as for the cable. Since the cables made so far are able to meet the pressure drop requirement comfortably, we have not encountered any problem in requiring the same flow admittance in the coil, despite some quite complex geometries (see next section).

IV. Magnets

Designations

Bending Magnets

Prefix C: C-magnet Width: in. (Arabic),
 H: H-magnet actual pole width
 P: Picture-frame Gap Height: in. (Roman)
 R: Radiussed ends to nearest integer.

Iron Length: in. (Arabic)

Suffix: M: Mineral-insulated / Field Strength, kG
 R: Radiation-hardened
 Conventional if omitted e.g., H18III21/20

Quadrupoles

Diameter: in.

Q (quadrupole) Iron length: in. / pole tip
 E: ellipt. beam tube Suffix as above / field, kG
 N: narrow (3 x bore) e.g., 8QN16M/7

LAMPF Switchyard

The magnets for the LAMPF switchyard have been briefly described.⁵ These magnets are now in operation, and Fig. 5 shows the switchyard.

LAMPF Experimental Area

Higher power magnets are required in the experimental area, although the medium-energy operation places the emphasis on field quality rather than high field strength. Bending magnets generally are 15-16 kG, and quadrupoles up to 9 kG at the pole tip. The radiation environment for magnets in the target cells is estimated at 10^{11} - 10^{12} rad/yr.

Bending Magnets. Most experimental area bending magnets use 0.75" sq hollow m.i. cable (Table 6) rated at 1800A in lengths up to 220 ft, or at 2000A in lengths up to 100 ft. The LAMPF cooling water system is 300 psi.

These magnets vary in complexity: Fig. 6 shows a PR24VI37M/15, with adjustable shoes on the field clamp to trim the effective field boundary to the required radius. The saddle coils have one concave and one convex end, which require care in winding to avoid twisting the cable at the bends.

Pole shaping is used on the C7III32M/16 (Fig. 7) to improve field uniformity. See Section V.

Quadrupoles. Quadrupoles use the 0.53" sq hollow m.i. cable (Table 5). Their mechanical design depends heavily on the LBL design of narrow quadrupoles.⁶ Provided that the basic pole blocks for these magnets are made rectangular initially (Blanchard grinding is recommended) the magnet assembly requires little adjustment to produce symmetry and so a low sextupole component.

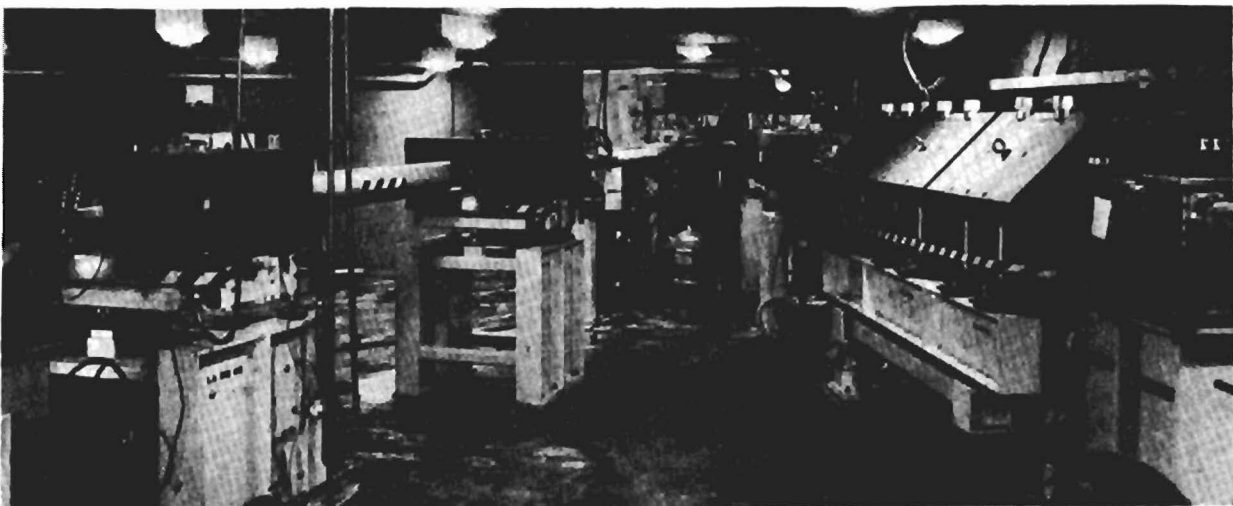


Fig. 5. LAMPF switchyard, looking upstream. "Straight-thru" line to Area A on left; line X (spectrometer and Areas B and C) on right.

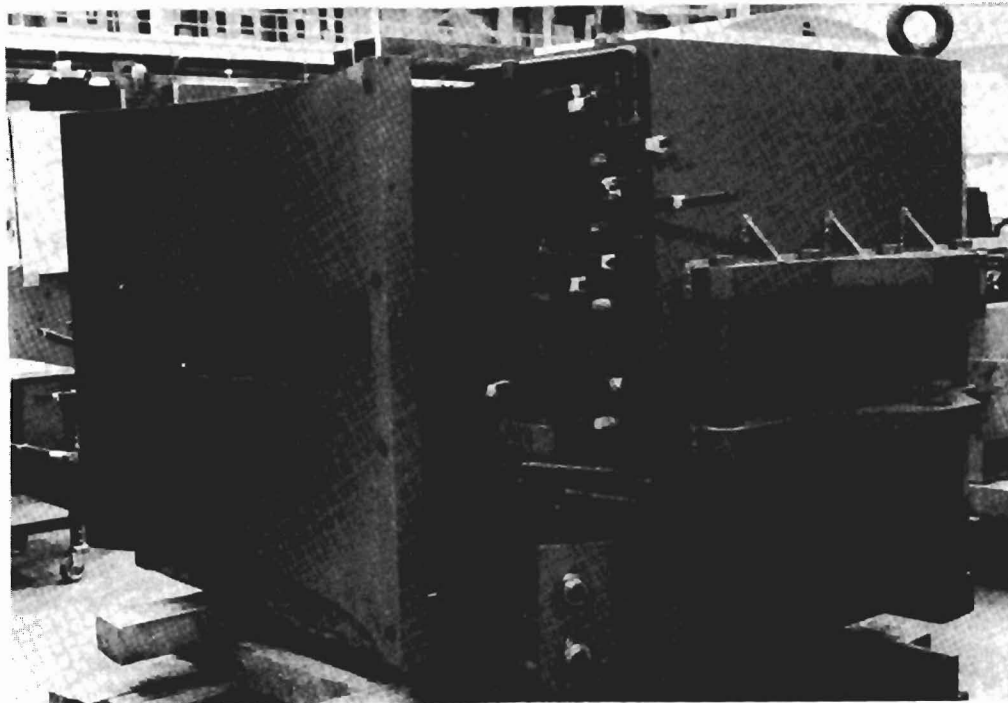


Fig. 6. PR24VI37M/15 magnet with 0.75" sq m.i. cable, as received from the manufacturer.

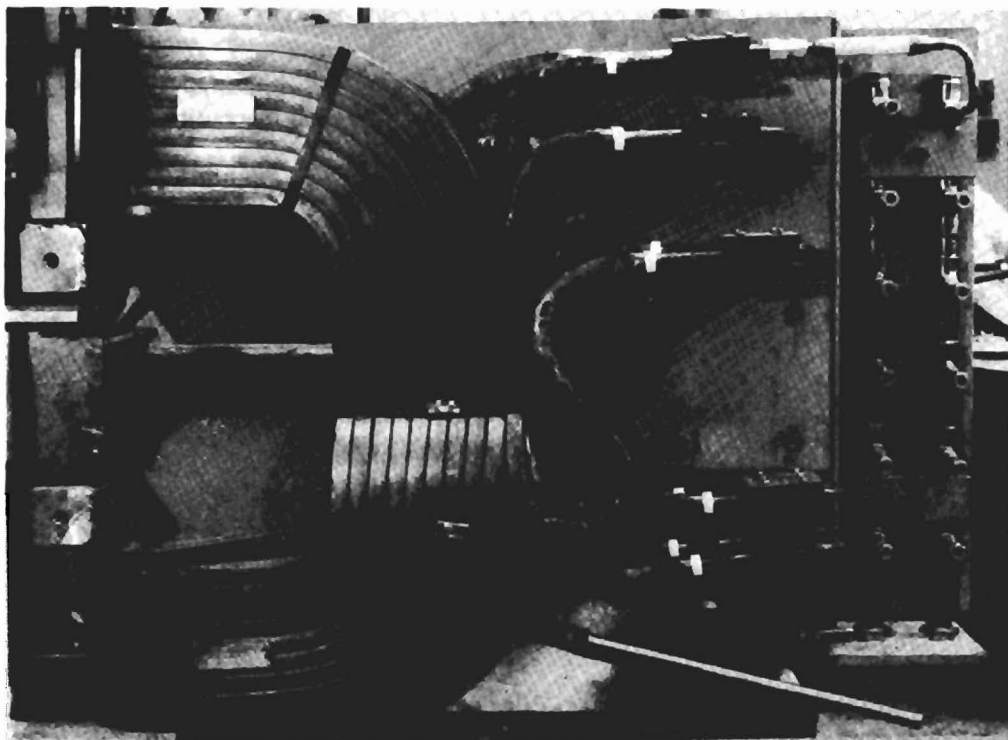


Fig. 7. C7III32M/16 magnet, with 0.75" sq m.i. cable. Some seals and connectors installed, plus one water insulator and one terminal plate.

Pole shaping for these quadrupoles was done at LASL (see Section V), and the pole-end chamfering to reduce duodecapole to an acceptable level was performed at LASL as described in a companion paper.⁷ The measured values obtained for two sizes of quadrupoles are given in Table 9.

TABLE 9.

Magnet	Current A	Pole Tip Field kG	Integrated Harmonics as % of n = 2		
			n = 3	n = 6	n = 10
8QN16M/7	750	6.7	0.033	< 0.1	0.026
11QN22M/9	750	9.1	0.022	0.07	0.01

Costs. To illustrate the contention that the overall cost of a mineral-insulated magnet is not very different from a conventional one, we list in Table 10 the costs of magnets procured for LAMPF. Magnets with an M before the slash are mineral-insulated; those without generally have epoxy-fiberglass insulated coils. Note, however, that the cost of applying seals and insulators to the mineral-insulated coils is not included in these costs. LASL experience to date indicates that about a man-month of labor is required in addition to the hardware, making this operation cost about \$2,000 per magnet, for directly-cooled magnets. Magnets in the table are listed in order of increasing weight, but there is no indication of the quality of the magnetic field, an important factor.

Magnet Characteristics. Two features of m.i. cable wound magnets are worth mentioning. First, the sheath surrounding the conductor acts as a transformer secondary of low impedance, so that ripple voltage from a power supply will cause ripple current to flow in the coil to an extent not seen in conventional coils. However, the balancing sheath current suppresses the ripple in the magnetic field to the same level as in a conventional magnet.

The sheath also serves as a shield for electrical noise (if an SCR power supply is used, for instance). This can be a decided advantage if counting equipment is in the vicinity: obviously, the magnet leads have to be shielded as well, and at LAMPF many of these are also m.i. cable.

V. Pole Shaping


General

Two techniques have been used to determine pole shapes for the magnets described here. Shims for low-field bending magnets were derived by experiment, and the same shims were conformally transformed to produce poles for the 2" quadrupoles.

Alternately, the magnetostatic design program POISSON was used in an inversion program, MIRT,⁸ to optimize the pole profile in dipole geometry, and then transform this optimized pole, if required, into quadrupole geometry. Thus, the two methods are basically similar, the first being empirical, while the second, sophisticated, method uses a CDC 6600 computer. However, it may be noted in what follows that the first method was used primarily for the low-field switchyard magnets, while the latter was used for the higher-field experimental area magnets. While measurements on the switchyard magnets are now completed, those on the larger magnets are only now under way.

Empirical Approach

Bending Magnets. Reference 5 gave one experimentally-derived shim-anti-shim combination, which was used on a LAMPF switchyard bending magnet, the H10III69M/4. Figure 8 gives the measured field distribution from another pole shape, at roughly 4 kG and 2 kG. Also shown is the adjusted $\int B \cdot d\ell$ scan across the magnet, showing the effect of the end shims used to correct for the fall-off at the corners. These end shims are pieces of low-carbon sheet steel empirically chosen, and bolted

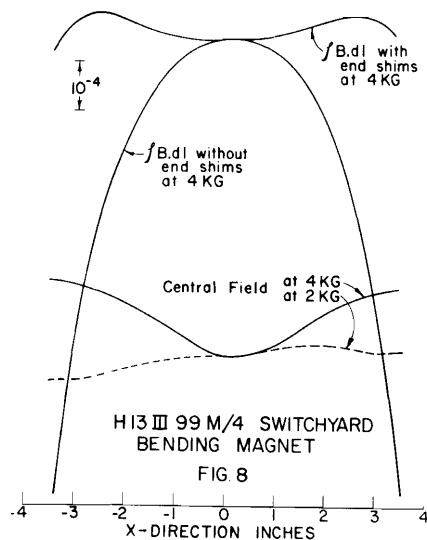

to the pole ends. Their thickness varies from 0.028 in. to 0.104 in., and length (i.e., across the magnet width) from 1 in. to 6 in. Their outer sides are aligned with the pole edge, and the side nearest the gap tapers away from the pole face to give some smoothing of the effect from stacked shims. Figure 9 shows a typical shim stack and the pole contour. It may be noted here that shimming as illustrated here, can only be done with low-field magnets. At higher fields the shim corners saturate, changing the field distribution.

TABLE 10

MAGNET PROCUREMENT COSTS


Magnet	Designation	No.	Weight (lb)	Cost (\$)	\$/lb
1° Bend, lines B & C	H9II9R/4	5	400	2,618	6.55
Inj. 2.5" Triplet	2Q5/1	1	600	3,650†	6.08
805 2" Quad. Doublets	2Q3/8	110	712	3,355†	4.71
Inj. 3" Triplets	3Q6/1	2	950	3,285†	3.46
Line "B" 4" Quads.	4Q12/5	6	957	2,950†	3.08
Inj. ± 30° Bend.	CW6II16/2.5	1	1,150	4,550†	3.96
Inj. 3" Quadruplets	3Q6/1	2	1,150	3,795†	3.30
Inj. 45°-20° Bend.	CW6II16/2.5	1	1,340	6,105†	4.555
Swyd. 2" Doublet	2Q19M/6	2	1,500	9,525	6.35
Inj. ± 45° Bend.	HW6II16/4	1	1,500	5,755†	3.84
Swyd. 2" Triplet	2Q9I9M/6	2	1,530	11,470	7.50
4° Bend, lines B & C	H9II38R/4	2	1,955	5,843	2.99
HRS quadrupole	8QE18/3	1	2,400	12,121	5.05
Swyd. 2° Bend.	H22III17M/4	5	3,500	6,982*§	1.99
Swyd. 6" Quad.	6Q22M/5	7	3,900	12,928§	3.31
Trans. 45° Bend.	H6II46/10	1	4,000	13,900†	3.48
8" narrow Quad.	8QN16M/7	4	4,020	11,279ψ§	2.80
Line "C" 6" Quad.	6Q29R/7	9	4,030	8,350	2.07
8" narrow Quad.	8QN16M/10	2	4,580	11,636ψ§	2.54
HRS quadrupole	10QE27/9	1	5,813	18,937	3.26
12" Danby Quads.	12Q15/9	12	6,200	12,676	2.04
Swyd. 8° Bends.	H10III69M/4	3	7,100	13,805*§	1.94
Line B "C" Bends.	C7III32M/15	5	8,200	10,202ψ§	1.24
EPICS quadrupole	12QE18/12	3	11,000	20,230	1.84
Swyd. 12° Bends.	H13III99M/4	3	13,700	16,837*§	1.23
11" narrow Quads.	11QN22M/9	2	13,800	21,087ψ§	1.53
Muon Channel Quads.	12QE20R/8	9	15,500	22,397ψ	1.44
Muon "C" Bends	C32XI30R/7	3	20,000	30,739ψ	1.54
LEP Epoxy Bend	PR20VI34/15	2	23,000	29,018	1.26
P ³ Bend	C12VI34M/15	1	28,800	33,575§	1.17
EPICS Model	H18III21/20	1	29,000	29,167*†	1.005
57° Bends.	H10II130/16	2	30,000	103,627*	3.45
Target cell Triplets	8&11QNM/7&9	9	30,800	53,542ψ§	1.74
LEP Bends.	PR24VI37M/15	2	40,000	49,147	1.22
High Resolution Spectrometer	H26X180/19	2	260,000	289,003ψ*	1.11

† includes vendor design

ψ LASL supplied conductor, incl. in cost


* LASL supplied steel, incl. in cost

§ does not include cable terminations & interlocks

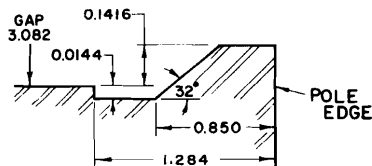

SHIM-ANTISHIM, H13 III 99 M/4

Quadrupoles. Quadrupole poles may be derived from bending magnet poles by conformal transformation, and Fig. 10 shows a pole shape for a 2" bore quadrupole, 2Q19M/6 designed by the $x = X^2$ transformation from the H10III69M/4 bending magnet shim.⁵ Table 11 gives the measured harmonics for this quadrupole with a 0.3 in. x 45° chamfer at the pole ends.

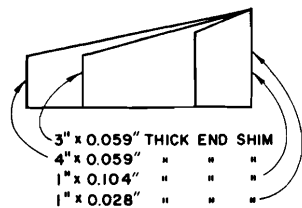

POLE SHIMS
FIG. 9

TABLE 11.

Magnet	Current A	Pole Tip Field kG	Integrated Harmonics as % of n = 2		
			n = 3	n = 6	n = 10
2Q19M/6	100	5.2	0.025	0.019	0.242
	50	2.7	0.01	0.03	0.239


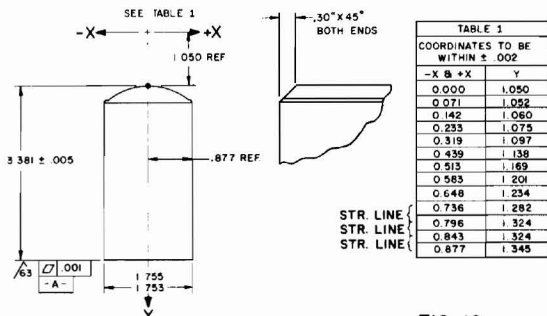


FIG. 10
2Q 19 M/6
POLE

NOTES
ALL FOUR POLE FACES FOR ANY MAGNET SHALL BE MACHINED TOGETHER, AND THE UPSTREAM END OF ALL POLES SHALL BE IMPRESSION STAMPED FOR IDENTIFICATION

Figure 11 shows the "adjustable box" construction used in the switchyard quadrupoles to achieve close symmetry tolerances: 0.004 in. on bore diameters and 0.002 in. between adjacent poles in the 6" bore quadrupole, and 0.001 in. (as shown in Fig. 12) for both measures in the 2" bore quadrupoles.

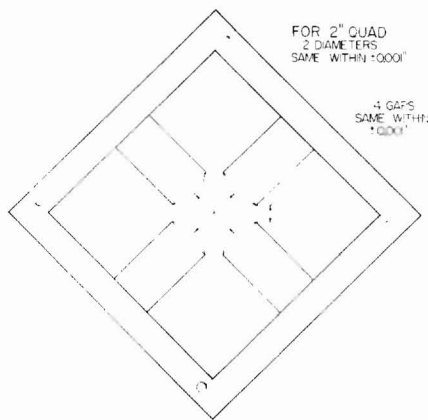

QUADRUPOLE SECTION
FIG. 11

A number of methods have been used to produce the shaped poles required: template-following planing, shaped milling cutters and planing with a variety of shaped tools to match a template. All seem to be satisfactory for the ±0.002 in. tolerance on the pole tip contour.

Beam Tubes. All beam tubes in the LAMPF switchyard quadrupole magnets are seamless austenitic stainless steel; in the bending magnets, the rectangular beam tubes have the welds well away

from the "good field" region. We have measured field perturbations of a part in 10^4 due to welds in 304 stainless steel made with no filler. If a filler rod is used, the perturbation is larger.

MIRT

More sophisticated pole shaping may be done with the help of computer-based magnetostatic programs. TRIM⁹ and POISSON solve the 2-dimensional field equations for arbitrarily-shaped iron boundaries, and can accommodate not only the conductors, but also differing permeabilities in sections of the magnet. These programs have the advantage over the techniques in the previous section that smooth-contour shims can be incorporated, making saturation less of a problem. The inversion program⁸ incorporated in MIRT is set up to allow the designer to vary the pole contour in designated areas to achieve the field uniformity required. The 3" gap, 16kG, C-magnet (C7III32M/16) has a calculated field uniformity of 0.5G over the 2 in. beam trajectory. Figure 7 is a photograph of this magnet nearing completion. Table 12 is the coordinate table for an 11 in. bore quadrupole, 11QN22M/9, with negligible $n = 6$ (duodecapole).

TABLE 12.

Coordinate Table, 11QN22M/9
(Tolerance = ±0.002)

X	Y	X	Y
2.140	7.000	3.305	5.294
2.224	6.830	3.180	5.052
2.417	6.633	3.363	4.778
2.620	6.325		
2.684	6.044	3.568	4.503
		3.800	4.227
2.782	5.774	4.008	4.008
2.904	5.532		Pole Centerline

VI. Acknowledgments

Many of the handling and terminating techniques for m.i. cables described here are the result of joint efforts and discussions at Pyrotenax of Canada Ltd., and at LASL. The development work on producing hollow m.i. cable owes a great deal to the efforts of Mr. Sid Walker, plant manager of Pyrotenax. The seal application has been developed and implemented by LASL technicians under the capable direction of Ted Montoya.

The MIRT computations were made by Ron Yourd, now of LBL, while at LASL. Finally, the measurements reported here were taken by the LAMPF section directed by Wm. Hassenzahl.

References

1. L. R. Glasgow and R. J. Burleigh, Nucl. Instr. & Methods 18, 19, 576-581 (1962).
2. A. Harvey and S. A. Walker, IEEE Trans. Nucl. Sci. NS-16, No. 3, 611 (1969).
3. A. Harvey, Proc. 1970 Linac Conf., National Accelerator Laboratory, Batavia, Ill., p. 709.
4. W. O. Brunk, C. A. Harris, and D. B. Robbins, IEEE Trans. Nucl. Sci. NS-18, No. 3, 887 (1971).
5. A. Harvey and R. D. Turner, IEEE Trans. Nucl. Sci. NS-18, No. 3, 892 (1971).
6. K. H. Lou, J. M. Hauptman, and J. E. Walter, "High-Quality Narrow Quadrupole Magnets," Lawrence Berkeley Laboratory Report, UCRL-18558 (1967).
7. W. V. Hassenzahl, "An Algorithm for Eliminating the Duodecapole Component in Quadrupole Magnets," these Proceedings.
8. K. Halbach, Proc. 2nd Int. Conf. on Magnet Technology, Oxford, 1967, p. 47
9. J. S. Colonias and J. H. Dorst, 1st Int. Symp. on Magnet Technology, SLAC, CONF-650922, 1965, p. 188.